

Calibration Certificate

Certificate Number 2021013664

Customer:

SGS Del Peru S.A.C.

Av. Elmer Faucett Nro. 3348, Callao.

Lima, Perú



Model Number CAL200
Serial Number 19459
Test Results Pass
Initial Condition As Manufactured
Description Larson Davis CAL200 Acoustic Calibrator

Procedure Number D0001.8386
Technician Scott Montgomery
Calibration Date 25 Oct 2021
Calibration Due
Temperature 23 °C ± 0.3 °C
Humidity 35 %RH ± 3 %RH
Static Pressure 101.2 kPa ± 1 kPa

Evaluation Method The data is acquired by the insert voltage calibration method using the reference microphone's open circuit sensitivity. Data reported in dB re 20 µPa.

Compliance Standards Compliant to Manufacturer Specifications per D0001.8190 and the following standards:
IEC 60942:2017 ANSI S1.40-2006

Issuing lab certifies that the instrument described above meets or exceeds all specifications as stated in the referenced procedure (unless otherwise noted). It has been calibrated using measurement standards traceable to the SI through the National Institute of Standards and Technology (NIST), or other national measurement institutes, and meets the requirements of ISO/IEC 17025:2017. Test points marked with a ‡ in the uncertainties column do not fall within this laboratory's scope of accreditation.

The quality system is registered to ISO 9001:2015.

This calibration is a direct comparison of the unit under test to the listed reference standards and did not involve any sampling plans to complete. No allowance has been made for the instability of the test device due to use, time, etc. Such allowances would be made by the customer as needed.

The uncertainties were computed in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). A coverage factor of approximately 2 sigma (k=2) has been applied to the standard uncertainty to express the expanded uncertainty at approximately 95% confidence level.

This report may not be reproduced, except in full, unless permission for the publication of an approved abstract is obtained in writing from the organization issuing this report.

Standards Used

Description	Cal Date	Cal Due	Cal Standard
Larson Davis Model 2900 Real Time Analyzer	04/01/2021	04/01/2022	001051
Agilent 34401A DMM	03/02/2021	03/02/2022	002588
Microphone Calibration System	02/24/2021	02/24/2022	005446
1/2" Preamplifier	08/26/2021	08/26/2022	006506
Larson Davis 1/2" Preamplifier 7-pin LEMO	08/09/2021	08/09/2022	006507
1/2 inch Microphone - RI - 200V	09/23/2021	09/23/2022	006511
Hart Scientific 2626-H Temperature Probe	02/04/2021	08/04/2022	006767
Pressure Transducer	06/28/2021	06/28/2022	007310

LARSON DAVIS - A PCB PIEZOTRONICS DIV.
1681 West 820 North
Provo, UT 84601, United States
716-684-0001



Output Level

Nominal Level [dB]	Pressure [kPa]	Test Result [dB]	Lower limit [dB]	Upper limit [dB]	Expanded Uncertainty [dB]	Result
114	101.5	114.00	113.80	114.20	0.14	Pass
94	101.2	94.01	93.80	94.20	0.15	Pass

-- End of measurement results--

Frequency

Nominal Level [dB]	Pressure [kPa]	Test Result [Hz]	Lower limit [Hz]	Upper limit [Hz]	Expanded Uncertainty [Hz]	Result
114	101.5	1,000.00	993.00	1,007.00	0.20	Pass
94	101.2	1,000.01	993.00	1,007.00	0.20	Pass

-- End of measurement results--

Total Harmonic Distortion + Noise (THD+N)

Nominal Level [dB]	Pressure [kPa]	Test Result [%]	Lower limit [%]	Upper limit [%]	Expanded Uncertainty [%]	Result
114	101.5	0.33	0.00	2.00	0.25 ‡	Pass
94	101.2	0.39	0.00	2.00	0.25 ‡	Pass

-- End of measurement results--

Level Change Over Pressure

Tested at: 114 dB, 24 °C, 30 %RH

Nominal Pressure [kPa]	Pressure [kPa]	Test Result [dB]	Lower limit [dB]	Upper limit [dB]	Expanded Uncertainty [dB]	Result
108.0	107.9	-0.02	-0.25	0.25	0.04 ‡	Pass
101.3	101.5	0.00	-0.25	0.25	0.04 ‡	Pass
92.0	91.9	0.03	-0.25	0.25	0.04 ‡	Pass
83.0	83.1	0.03	-0.25	0.25	0.04 ‡	Pass
74.0	74.0	0.01	-0.25	0.25	0.04 ‡	Pass
65.0	64.9	-0.06	-0.25	0.25	0.04 ‡	Pass

-- End of measurement results--

Frequency Change Over Pressure

Tested at: 114 dB, 24 °C, 30 %RH

Nominal Pressure [kPa]	Pressure [kPa]	Test Result [Hz]	Lower limit [Hz]	Upper limit [Hz]	Expanded Uncertainty [Hz]	Result
108.0	107.9	0.00	-7.00	7.00	0.20 ‡	Pass
101.3	101.5	0.00	-7.00	7.00	0.20 ‡	Pass
92.0	91.9	0.00	-7.00	7.00	0.20 ‡	Pass
83.0	83.1	-0.01	-7.00	7.00	0.20 ‡	Pass
74.0	74.0	-0.01	-7.00	7.00	0.20 ‡	Pass
65.0	64.9	-0.02	-7.00	7.00	0.20 ‡	Pass

-- End of measurement results--

Total Harmonic Distortion + Noise (THD+N) Over Pressure

Tested at: 114 dB, 24 °C, 30 %RH

Nominal Pressure [kPa]	Pressure [kPa]	Test Result [%]	Lower limit [%]	Upper limit [%]	Expanded Uncertainty [%]	Result
108.0	107.9	0.32	0.00	2.00	0.25 ‡	Pass
101.3	101.5	0.33	0.00	2.00	0.25 ‡	Pass
92.0	91.9	0.32	0.00	2.00	0.25 ‡	Pass
83.0	83.1	0.33	0.00	2.00	0.25 ‡	Pass
74.0	74.0	0.34	0.00	2.00	0.25 ‡	Pass
65.0	64.9	0.36	0.00	2.00	0.25 ‡	Pass

-- End of measurement results--

Signatory: Scott Montgomery

LARSON DAVIS - A PCB PIEZOTRONICS DIV.
1681 West 820 North
Provo, UT 84601, United States
716-684-0001



 **LARSON DAVIS**
A PCB DIVISION




Model CAL200 Relative SPL vs. Temperature

Larson Davis Model CAL200 Serial Number: 19459

Model CAL200 Relative SPL vs. Temperature at 50% RH.

A 2559 Mic (SN: 2997) with a PRM901 Preamp (SN: 0201), station 21 was used to check the levels.

Test Date: 30 Sep 2021 4:13:54 PM

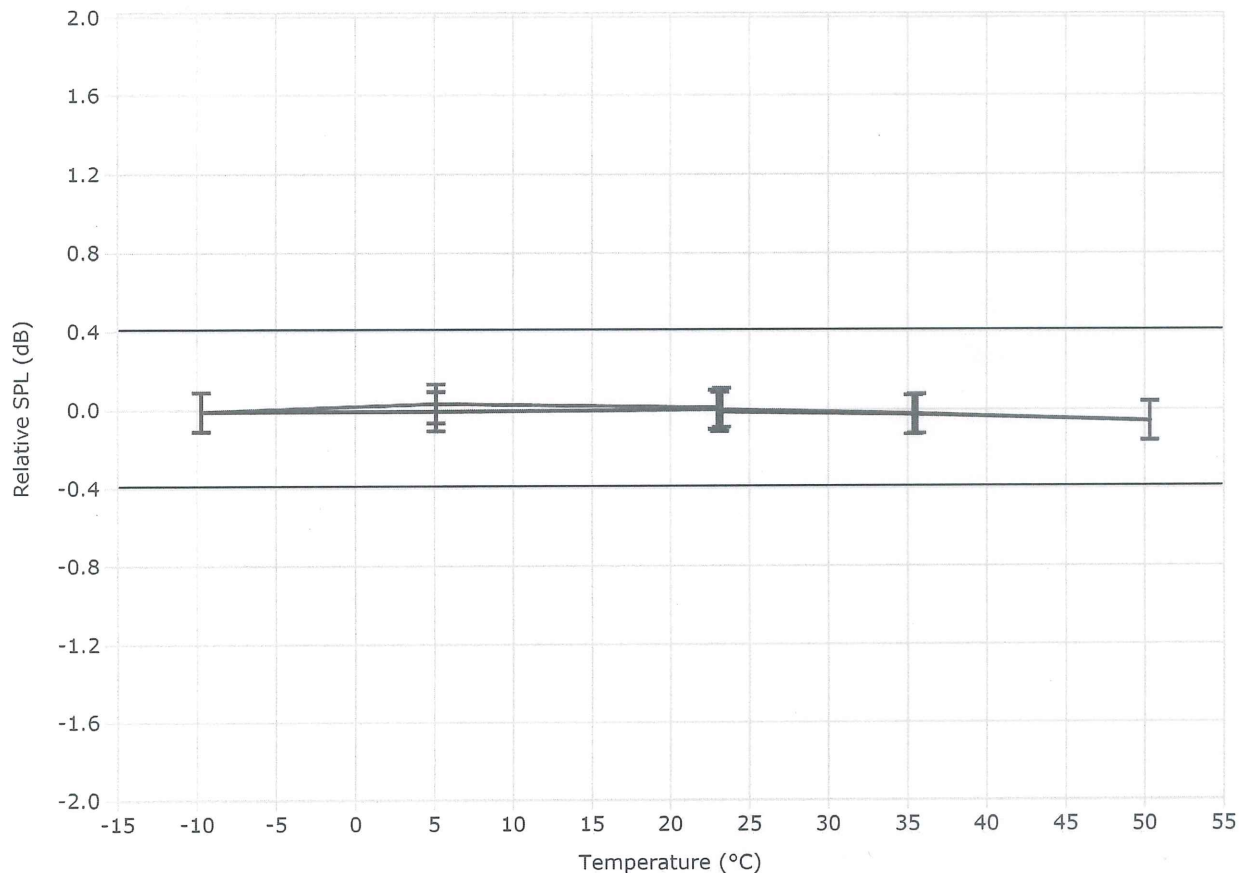

0.1dB expanded uncertainty at ~95% confidence level (k=2)

Sequence File: CAL250w200s.SEQ

Test Location: Larson Davis, a division of PCB Piezotronics, Inc.
1681 West 820 North, Provo, Utah 84601
Tel: 716 684-0001 www.LarsonDavis.com




Model CAL200 Relative Frequency vs. Temperature

Larson Davis Model CAL200 Serial Number: 19459

Model CAL200 Relative Frequency vs. Temperature at 50% RH.
A 2559 Mic (SN: 2997) with a PRM901 Preamp (SN: 0201), station 21 was used to check the levels.

Test Date: 30 Sep 2021 4:13:54 PM

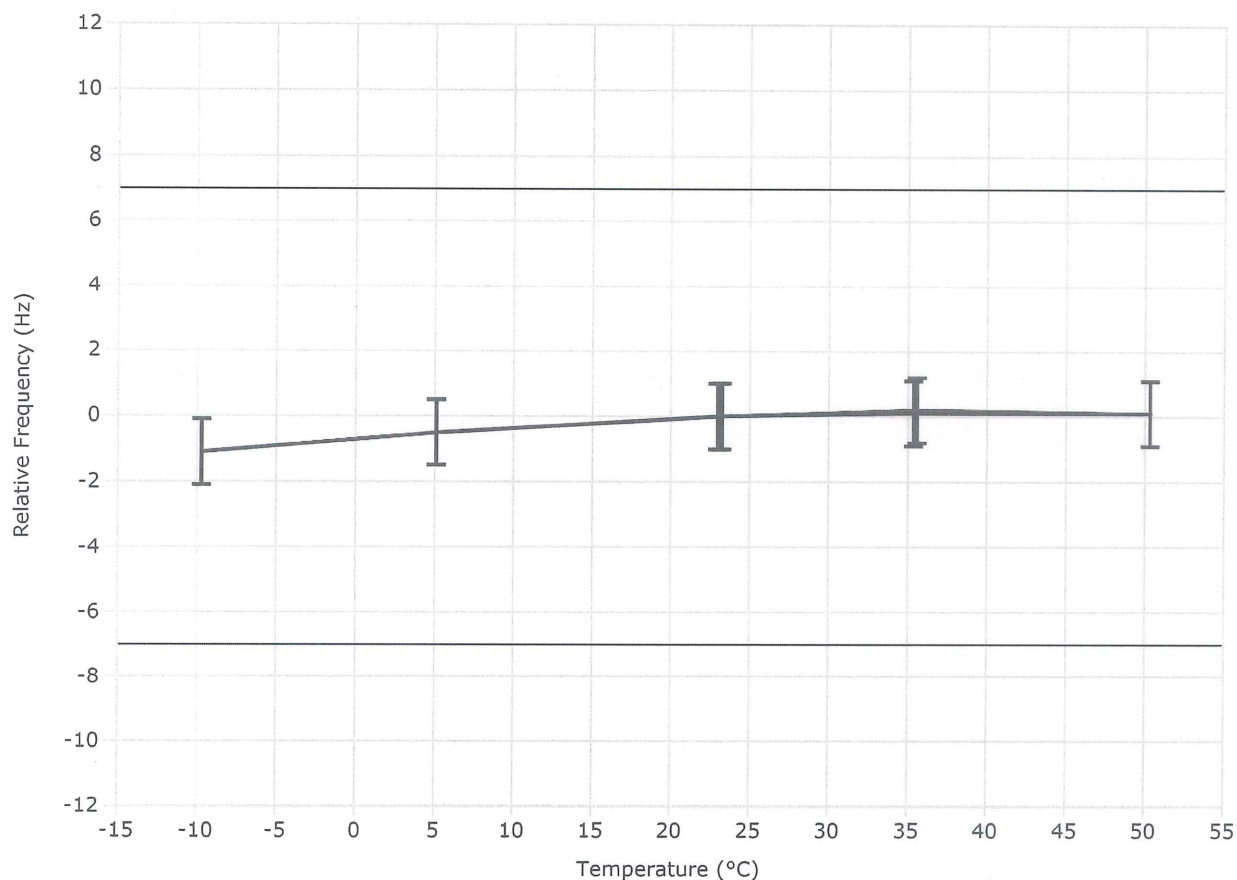

1.0 Hz expanded uncertainty at ~95% confidence level ($k=2$)

Sequence File: CAL250w200s.SEQ

Test Location: Larson Davis, a division of PCB Piezotronics, Inc.
1681 West 820 North, Provo, Utah 84601
Tel: 716 684-0001 www.LarsonDavis.com